


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: POLYETHYLENE GLYCOLS (PEG 300)

HPLC
Gradient

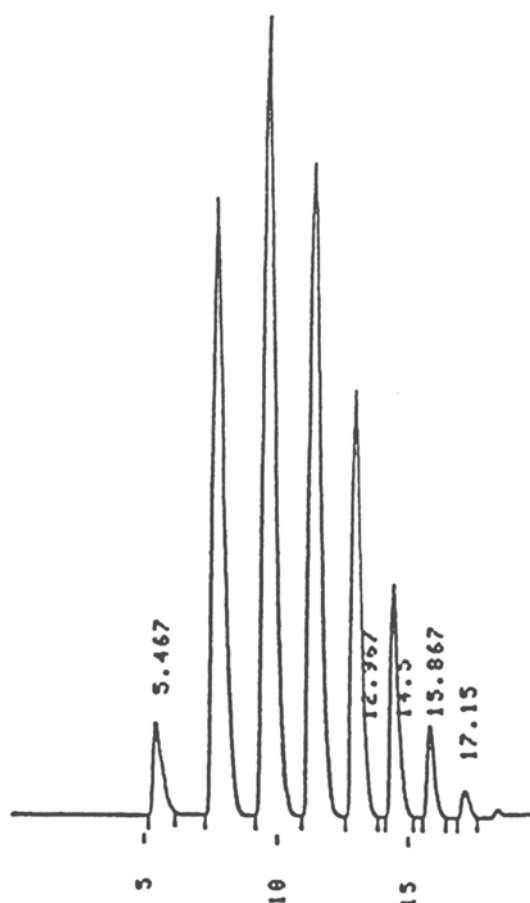

Gradient: Methanol/Water 10/90 to 90/10 in 30 min

CONDITIONS

Column	Zorbax TMS - 7 μ m 150 x 4.6 mm
Injected Volume	20 μ l (Injected Quantity 8 μ g)
Eluent	A: Methanol B: Water
Flow Rate	1.5 ml/min
Gas	Air
Pressure	2.5 Bars
Temperature	40° C

Analyzed By : LCBA 45100 Orleans FRANCE