


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: POLYETHYLENE GLYCOLS PEG 400

HPLC
Gradient

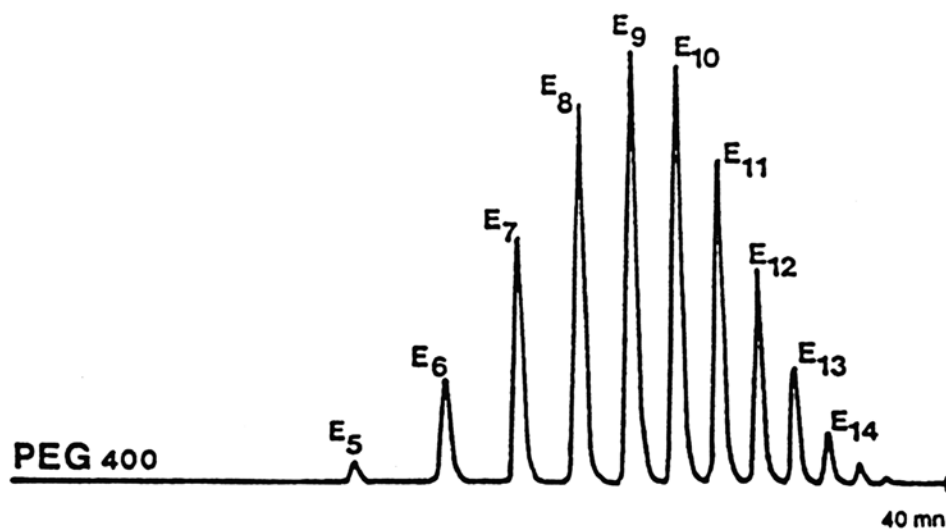

Gradient: Acetonitrile/Water 10/90 to 90/10 in 40 min

CONDITIONS

Column	<i>PLRPS - 5 μm 150 x 4.6 mm</i>
Injected Volume	<i>20 μl (Injected Quantity 10 μg)</i>
Eluent	<i>A: Acetonitrile B: Water</i>
Flow Rate	<i>1.5 ml/min</i>
Gas	<i>Air</i>
Pressure	<i>2.5 Bars</i>
Temperature	<i>40° C</i>

Analyzed By : LCBA 45100 Orleans FRANCE