


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: SUGARS (FROM TOBACCO)

HPLC

- 1: Fructose
- 2: Glucose
- 3: Sucrose

(Aqueous sample purified by Hamilton Cartridge)

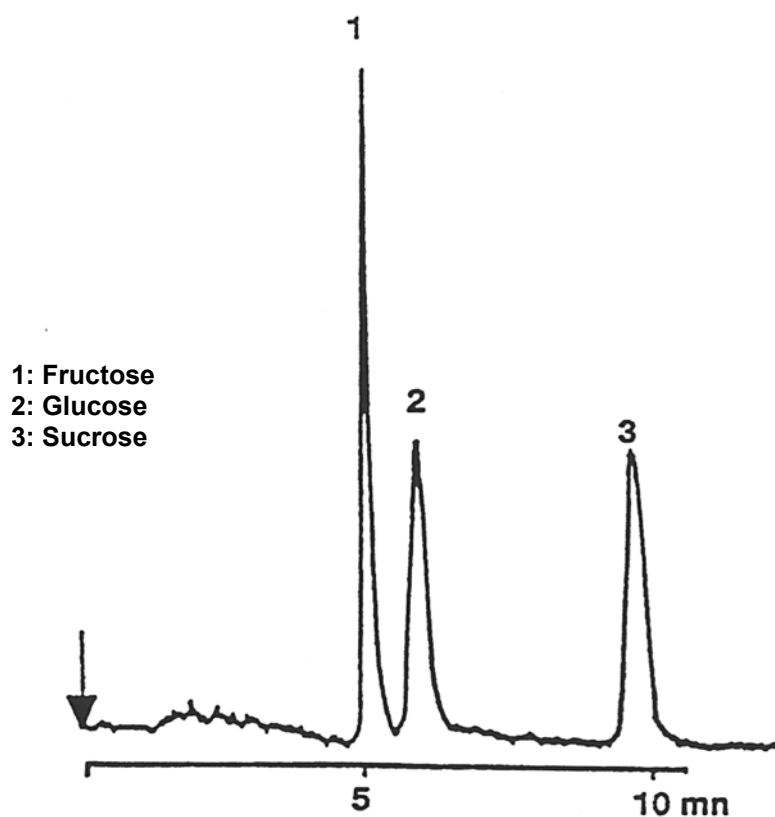

CONDITIONS

Column	<i>Nucleosil NH₂</i> <i>250 x 4.6 mm</i>
Injected Volume	<i>20 µl</i>
Eluent	<i>Acetonitrile/Water (80/20)</i>
Flow Rate	<i>1.0 ml/min</i>
Gas	<i>Air</i>
Temperature	<i>45° C</i>

Analyzed by : LCBA 45100 Orleans FRANCE