


SEDEX Low Temperature Evaporative Light Scattering Detector

SAMPLE: UREA 13 (Batch N° X3201)

HPLC
Gradient

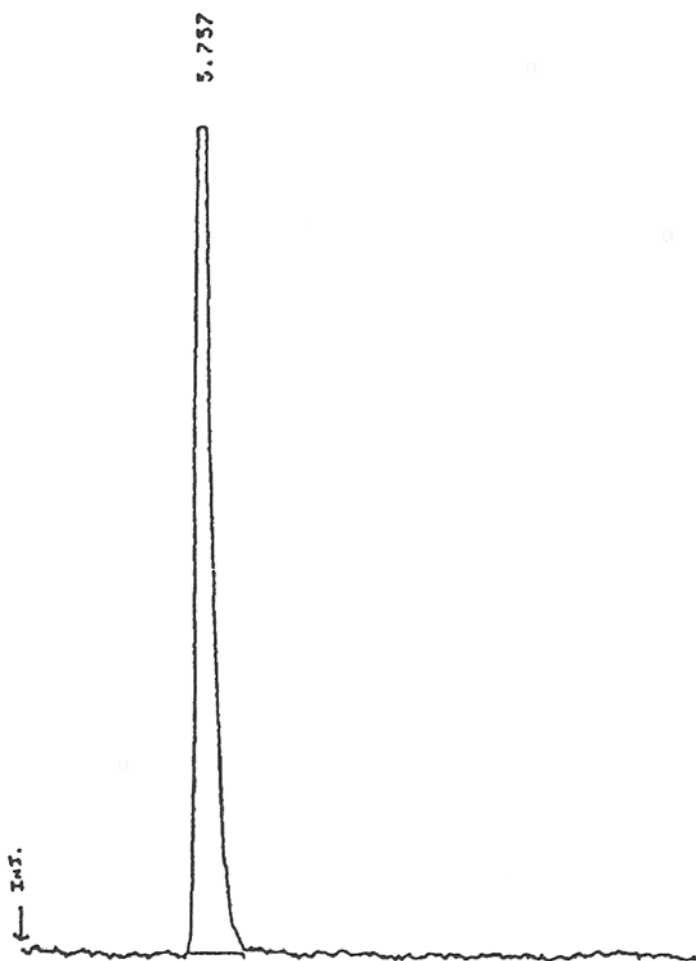

CONDITIONS

Column	<i>Waters Carbohydrate 250 x 4.6 mm</i>
Injected Volume	<i>15 µl (3 mg/ml)</i>
Eluent	<i>Acetonitrile/Water (95/5)</i>
Flow Rate	<i>1.0 ml/min</i>
Pressure	<i>2 bars</i>
Gas	<i>Helium</i>
Temperature	<i>60° C</i>

Analyzed by: CE Saclay Molecules Marquees 91191 Gif Sur Yvette FRANCE

S.E.D.E.R.E.
PARC VOLTA - BP 27
9, rue Parmentier
94141 Alfortville Cedex FRANCE

Application #78